

INSTRUMENT APPROACH CHART - ICAO PLAN VIEW SCALE:1:350 000


BRØNNØYSUND

BRØNNØY

RNAV(GNSS) -A

TRANSITION ALTITUDE
7000

ATIS: 135.900	AD ELEV: 25	
APP: 127.900		DIST IN NM
AFIS: 119.600		ELEV, ALT AND HGT IN FT
VDF: 119.600	CIRCLING HGT RELATED TO AD ELEV	
	BEARINGS ARE MAGNETIC - VAR 3.6 ° E (2015)	

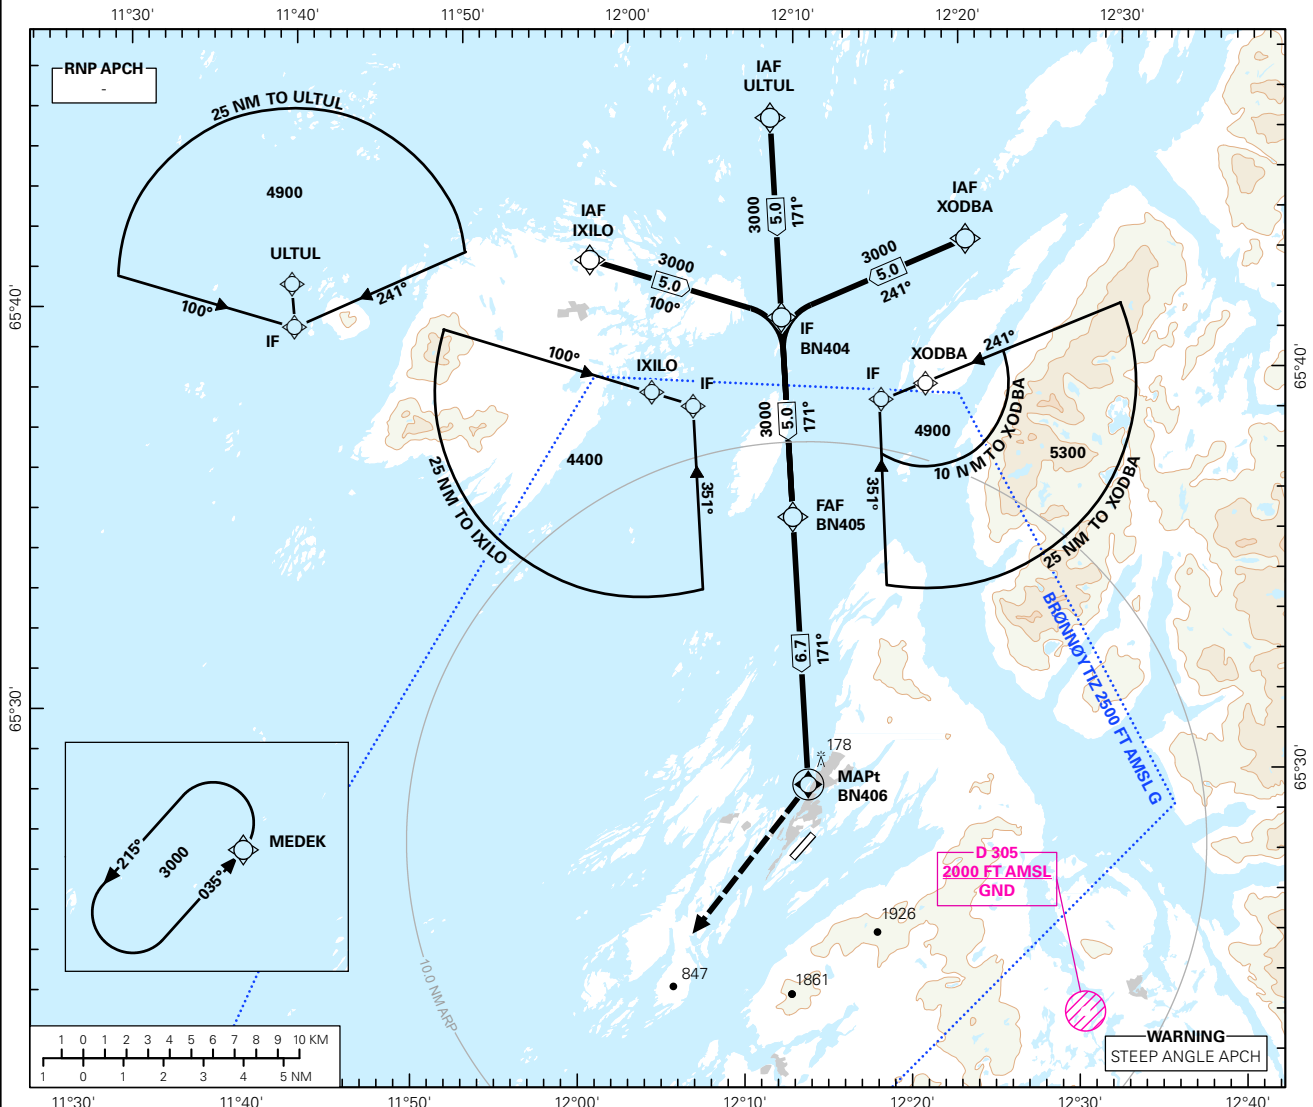


DIST TO BN406	8	7	6	5	4	3	2	1
ALT (HGT)	-	-	2740 (2715)	2360 (2335)	1990 (1965)	1610 (1585)	1230 (1205)	850 (825)

MISSED APCH:
AT MAPt TURN RIGHT DCT MEDEK.
ENTER MEDEK HLDG CLIMBING
TO 3000.

NOTE:
DESCENT GRADIENT CALCULATED
FROM BN405 TO BN406.

NOTE:
MAX 130 KT IAS IN INITIAL TURN.

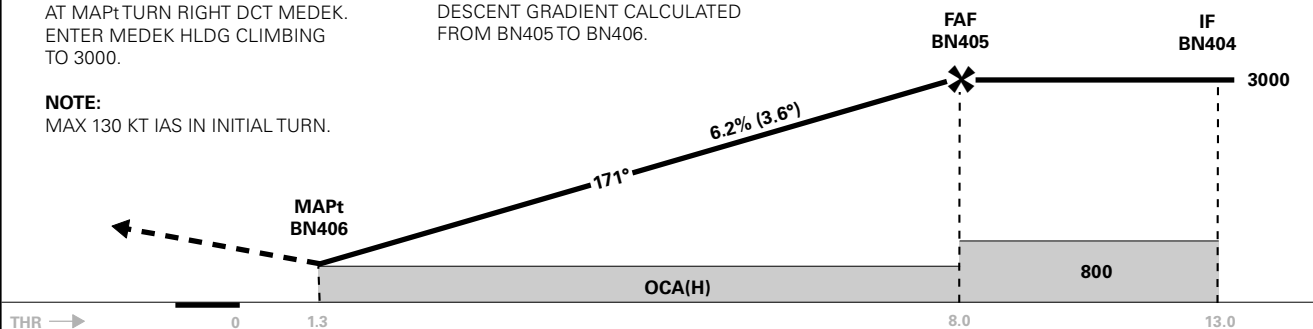

CAT OF ACFT	A	B	C	D	FINAL APCH	DIST FAF - MAPt: 6.7				
OCA(H)	-	-	-	-	SPEED	KT	70	90	100	120
STRAIGHT - IN	-	-	-	-	TIME	MIN:SEC	05:45	04:28	04:02	03:21
CIRCLING	2.5%*	1050 (1025)	-	-	ROD	FT/MIN	440	565	630	755
	3.5%*	470 (445)	740 (715)	-						

NOTE: CIRCLING W OF AD ONLY. *MNM MISSED APCH CLIMB GRADIENT.

RECOMMENDED RNAV PROCEDURE CODING

ENBN RNAV(GNSS)-A										
Serial Number	Path Descriptor	Waypoint Identifier	Fly-over	Course °M(°T)	MAG VAR	DIST (NM)	Turn Dir	ALT (FT)	Speed (KT)	VPA/ TCH
010	IF	IXILO	-	-	-	-	-	A3800+	-	-
020	TF	BN404	-	-	-	5.0	-	A3000+	-	-
010	IF	XODBA	-	-	-	-	-	A5200+	-	-
020	TF	BN404	-	-	-	5.0	-	A3000+	-	-
010	IF	ULTUL	-	-	-	-	-	A4900+	-	-
020	TF	BN404	-	-	-	5.0	-	A3000+	-	-
030	TF	BN405	-	-	-	5.0	-	A3000+	-	-
040	TF	BN406	Y	-	-	6.7	-	-	-	-
050	DF	MEDEK	-	-	-	-	-	A3000	K130-	-
060	HM	MEDEK	-	035(038.8)	-	1 MIN	L	A3000+	-	-

Note: Recommended RNAV procedure coding is based on ARINC 424-15 and is provided solely to indicate which procedure design protection areas were used in the Instrument Flight Procedure Design process.